


FRISHAUF, HOLTZ, GOODMAN, LANGER & CHICK, P.C.  
ATTORNEYS AT LAW

767 THIRD AVENUE, NEW YORK, N.Y. 10017-2023

Express Mail Mailing Label  
No.: EL 396 045 137 US

Date of Deposit: February 1, 2000

I hereby certify that this paper is being deposited with the United States Postal Service "Express Mail Post Office to Addressee" service under 37 CFR 1.10 on the date indicated above and is addressed to the Commissioner of Patents and Trademarks, Washington, D.C. 20231

  
Barbara Villani

Attorney Docket No. 00048/LH

Pursuant to 37 CFR 1.53(b), transmitted herewith for filing is the patent application of

**Inventor(s):** Masaru SUDO  
Kanichi MATSUMOTO
**Title:** "ENDOSCOPE IMAGE SENSING METHOD AND APPARATUS"**Priority Claim** (35 U.S.C. 119) is made, based upon:

Japan No. 11-027354 February 4, 1999

**Enclosed herewith are:**

- ☒ Specification (Description, Claims, Abstract): Pages 1 - 34; Number of claims 1 - 26
- ☒ Declaration and Power of Attorney ☒ executed; ☐ unexecuted (supplied for information purposes)
- ☒ 9 Sheets of drawings, Figures 1 - 14 ☒ Formal ☐ Informal
- ☒ Assignment and "Patents" Recordation Form Cover Sheet (PTO-1595) AND \$40. RECORDATION FEE.
- ☐ Certified copy (ies) of priority document(s) identified above
- ☒ Information Disclosure Statement; ☒ Form PTO-1449
- ☐ Preliminary Amendment
- ☐ Verified Statement(s) Claiming Small Entity Status
- ☒ Receipt Postcard

	Number Filed			Number Extra		Rate		Calculations
Total Claims	<u>26</u>	-20 =		<u>6</u>		x \$18.00 =		\$ <u>108.00</u>
Independent Claims	<u>5</u>	-3 =		<u>2</u>		x \$78.00 =		\$ <u>156.00</u>
MULTIPLE DEPENDENT CLAIMS								\$ <u>          </u>
								\$ <u>          </u>
BASIC FEE								\$ <u>690.00</u>
Total of above Calculations								\$ <u>954.00</u>

To the extent not tendered by check, authorization is given to charge any fees under 37 CFR 1.16 and 1.17 during pendency of the application, or to credit any overpayment, to Deposit Account No. 06-1378. Duplicate copy of this letter is enclosed.

FRISHAUF, HOLTZ, GOODMAN, LANGER &amp; CHICK, P.C.

  
By: Robert F. Michal, Reg. No. 35,614  
for Leonard Holtz, Reg. No. 22,974

TITLE OF THE INVENTION

ENDOSCOPE IMAGE SENSING METHOD AND APPARATUS

BACKGROUND OF THE INVENTION

5 The present invention relates to an endoscope  
image sensing method and apparatus which are suitable  
for every observation region and realize color  
reproduction independent of the type of light source.

10 In general, for endoscope image sensing  
apparatuses for sensing an object by using an image  
sensing device such as a CCD (Charge Coupled Device),  
and obtaining a video signal by photoelectrically  
converting the sensed image data, it is important  
to ensure good color reproduction by eliminating  
variations resulting from different types of light  
15 sources and the like. To realize such good color  
reproduction, various types of adjustments such as  
white balance adjustment and black balance adjustment  
are performed.

20 For example, Jpn. Pat. Appln. KOKAI Publication  
No. 10-211166 discloses a technique associated with an  
endoscope image sensing apparatus which realizes good  
color reproduction by performing white balance and  
black balance adjustments. This apparatus is further  
characterized by preventing erroneous use of the white  
25 balance and black balance adjustments.

In an endoscope image sensing apparatus using an  
image sensing device such as a CCD as described above,

the luminance and color difference signals obtained by the image sensing device are arithmetically processed by using a uniquely defined matrix (to be referred to as a color matrix hereinafter) consisting of predetermined coefficients, thereby converting the signals into R, G, and B digital signals. The image represented by the signals is then displayed on the screen of a monitor or the like.

Endoscope image sensing apparatuses generally use various types of light sources. For example, FIGS. 8 to 10 respectively show the spectral characteristics of a xenon lamp, halogen lamp, and metal halide lamp. More specifically, FIG. 8 shows the spectral characteristics of a xenon lamp, which are similar to those of natural light and substantially uniform throughout the ultraviolet, visible, and infrared regions. FIG. 9 shows the spectral characteristics of a halogen lamp, which exhibit high output levels across the visible and infrared regions. FIG. 10 shows the spectral characteristics of a metal halide lamp, which exhibit high output levels in the visible region.

In endoscopic diagnoses, different color reproduction are desired depending on the observation regions. For this reason, as in the prior art, it is difficult to realize desired color reproduction by using only a uniquely defined color matrix regardless of the observation region or light source to be used.

If, for example, a one-chip CCD is used, a signal obtained by combining an output from the CCD having spectral sensibility characteristics like those shown in FIG. 11, an output from an infrared cut filter having spectral characteristics like those shown in FIG. 12, and an output from a light source having spectral characteristics like those shown in one of FIGS. 8 to 10 is input to an Y/C separation circuit.

If arithmetic operation is performed by using the uniquely defined color matrix described above after the signal is subjected to Y/C separation processing, the operation result varies depending on the light source used. As a consequence, the color reproduction yields different results.

For example, FIG. 13 shows the characteristics obtained by matrix operation using a xenon lamp as a light source. FIG. 14 shows the characteristics obtained by matrix operation using a halogen lamp as a light source. Obviously from the two graphs, the color reproduction result in one operation differ from that in the other operation.

#### BRIEF SUMMARY OF THE INVENTION

The present invention has been made in consideration of the above problems, and has as its object to provide an endoscope image sensing apparatus which can switch to a suitable color matrix in accordance with the type of observation region, the type of light

source used, or the like, and obtain good color reproduction corresponding to the type of observation region or the type of light source used.

In order to achieve the above object, according to the first aspect of the present invention, there is provided an endoscope image sensing apparatus comprising an image sensing section for obtaining an image signal by photoelectrically converting an object image, a conversion matrix section capable of changing a setting associated with a conversion matrix to a desired setting, the conversion matrix being used to convert the image signal, obtained by the image sensing section, into a video signal, by a predetermined matrix computation, and an input section for inputting information about a change in the setting associated with the conversion matrix.

According to the second aspect, there is provided an endoscope image sensing apparatus comprising an image sensing section for obtaining a image signal by photoelectrically converting an object image, a conversion matrix section for converting the image signal obtained by the image sensing section into a video signal by a predetermined matrix computation, a designating section for designating a change of a setting associated with conversion performed by the conversion matrix section, and a control section for changing a setting associated with the conversion

performed by the conversion matrix section on the basis of designation performed by the designating section.

According to the third aspect, there is provided an endoscope image sensing apparatus comprising a light  
5 source for irradiating an object with light, an image sensing section for obtaining a image signal by photoelectrically converting an object image, a conversion matrix section for converting the image signal obtained by the image sensing section into a video signal by  
10 a predetermined matrix computation, a communication section for performing serial communication with the light source, and a control section for performing serial communication with the light source through the communication section, receiving an identification  
15 signal associated with the light source, recognizing a type of light source, and changing a setting associated with conversion performed by the conversion matrix section on the basis of the type.

According to the fourth aspect, there is provided  
20 an endoscope image sensing apparatus comprising, a light source for irradiating an object with light, an image sensing section for obtaining an image signal by photoelectrically converting an object image, a conversion matrix section for converting the image  
25 signal obtained by the image sensing section into a video signal by a predetermined matrix computation, a white balance processing section for performing

white balance processing, and a control section for recognizing a type of light source on the basis of a magnitude of a gain coefficient set when the white balance processing is performed, and changing the setting associated with the conversion matrix section on the basis of the type of light source.

According to the fifth aspect, there is provided an endoscope image sensing method comprising the steps of obtaining an image signal by photoelectrically converting an object image, changing a setting associated with a conversion matrix to a desired setting, the conversion matrix being used to convert the image signal, obtained in the step of performing image sensing, into a video signal, by a predetermined matrix computation, and inputting information about a change in the setting associated with the conversion matrix.

Additional objects and advantages of the invention will be set forth in the description which follows, and in part will be obvious from the description, or may be learned by practice of the invention. The objects and advantages of the invention may be realized and obtained by means of the instrumentalities and combinations particularly pointed out hereinafter.

#### BRIEF DESCRIPTION OF THE SEVERAL VIEWS OF THE DRAWING

The accompanying drawings, which are incorporated in and constitute a part of the specification,

09496061-020100

illustrate presently preferred embodiments of the invention, and together with the general description given above and the detailed description of the preferred embodiments given below, serve to explain the principles of the invention.

FIG. 1 is a schematic view showing the arrangement of an endoscope image sensing apparatus of the present invention;

FIG. 2 is a block diagram showing the arrangement of an endoscope image sensing apparatus according to the first embodiment;

FIG. 3 is a block diagram showing the detailed arrangement of a color separation circuit 21 in FIG. 2;

FIG. 4 is a block diagram showing the arrangement of an endoscope image sensing apparatus according to the second embodiment;

FIG. 5 is a flow chart showing a matrix switching sequence in an endoscope image sensing apparatus according to the third embodiment;

FIG. 6 is a block diagram showing the arrangement of a modification of the first embodiment;

FIG. 7 is a view showing an example of how a menu is displayed on a monitor 37 in FIG. 6;

FIG. 8 is a graph showing the spectral characteristics of a xenon lamp;

FIG. 9 is a graph showing the spectral characteristics of a halogen lamp;



FIG. 10 is a graph showing the spectral characteristics of a metal halide lamp;

FIG. 11 is a graph showing the spectral sensibility characteristics of a CCD output;

5        FIG. 12 is a graph showing the spectral characteristics of an infrared cut filter;

FIG. 13 is a graph showing the spectral characteristics (with a xenon lamp ON) after matrix arithmetic processing; and

10        FIG. 14 is a graph showing the spectral characteristics (with a halogen lamp ON) after matrix arithmetic processing.

#### DETAILED DESCRIPTION OF THE INVENTION

15        The embodiments of the present invention will be described below with reference to the views of the accompanying drawing.

FIG. 1 is a conceptual view of an endoscope image sensing apparatus of the present invention. An overview of this apparatus will be described below.

20        As shown in FIG. 1, an endoscope image sensing apparatus 1 of the present invention is comprised of a camera head 2 incorporating a CCD, a scope 3 to which the camera head 2 is detachably connected, a light source section 4 for supplying illumination light to  
25        the scope 3, a camera control unit (to be abbreviated to CCU hereinafter) 5 serving as a processor for performing signal processing for the CCD incorporated

in the camera head 2, and a TV monitor 6 for displaying a standard video signal having undergone signal processing in the CCU 5.

5 The scope 3 is, for example, an optical endoscope having an insertion portion 7 in which an elongated, flexible image guide fiber (not shown) for transmitting an endoscopic image is inserted.

10 When the camera head 2 is detachably connected to the eyepiece of an operation portion 8 formed on the proximal end of the insertion portion 7 through an adaptor 2a, the endoscopic image sent to the eyepiece of the operation portion 8 through the image guide fiber (not shown) can be sensed by the camera head 2. A light guide cable 9 extends from the operation  
15 portion 8 of the scope 3. When the distal end of the light guide cable 9 is connected to the light source section 4, illumination light supplied from the light source section 4 is sent from the distal end of the scope 3 onto an object (not shown) through the light  
20 guide (not shown) inserted in the insertion portion 7.

When the endoscope image sensing apparatus 1 is used, the light guide cable 9 of the scope 3 is attached to the light source section 4. With this operation, although not shown, illumination light from  
25 the lamp of the light source section 4 passes through a stop, is focused by a lens, and strikes the opposing end face of the light guide. This illumination light

is sent to the scope 3 through the light guide, passes through the scope 3, and exits forward from the distal end of the scope 3. An object such as a body cavity of a patient is then irradiated with the illumination light. The light reflected by the object irradiated with the illumination light is formed into an image by the scope 3, and the object is sensed by the CCD in the camera head 2 through the scope 3.

In the camera head 2, the CCD is positioned at the focal plane of the image sensing lens so that an object image is formed on the image sensing plane of the CCD to be photoelectrically converted. This CCD is connected to the CCU 5 through a camera cable 12 which extends from the camera head 2 and in which a CCD driving signal transmission line and CCD output signal transmission line are inserted. An output signal from the CCD is sent to the CCU 5 to be subjected to various signal processes. The video signal output from the CCU 5 is sent to the TV monitor 6 to display an observation image of the object on the TV monitor 6.

In the arrangement described above, at the time of observation, the insertion portion 7 of the scope 3 is inserted into a body cavity, illumination light is supplied from the light source section 4 to the scope 3, and the endoscopic image sent to the eyepiece is sensed by the CCD of the camera head 2. This image signal is subjected to predetermined signal processing in the CCU

5 first, and then output to the TV monitor 6, thereby displaying an observation image on the TV monitor 6.

It is assumed that a one-chip color CCD is used in the present invention. Therefore, the video signal  
5 obtained by the CCD is separated into a luminance signal Y and chrominance signal C after predetermined processing. These signals are further separated into the luminance signal Y and color difference signals R-Y (Cr) and B-Y (Cb). By multiplying these signals by  
10 color matrix coefficients, R, G, and B signals can be obtained.

The color reproduction result of an observation image is determined by the above color matrix coefficients. The present invention is characterized in  
15 that a plurality of color matrixes are prepared, and suitable one of the color matrixes can be selected by manual or automatic switching operation using a switching means (to be described in detail later).

For example, in the present invention, three types  
20 of lamps, namely a xenon lamp, halogen lamp, and metal halide lamp, are assumed as light source sections 4. The spectral characteristics of these lamps have already been shown in FIGS. 8 to 10. As described above, since the different light source sections 4  
25 exhibit different characteristics, desired color reproduction may not be obtained by arithmetic processing which uses a single color matrix as in the prior

art. In consideration of this problem, according to the present invention, a color matrix can be selected in accordance with the type of light source to realize color reproduction independent of the light source.

5 This will be described in detail later in each embodiment.

Endoscope image sensing apparatuses according to the first to third embodiments using different methods of switching the above color matrix coefficients will  
10 be described in detail below.

The first embodiment of the present invention will be described first.

FIG. 2 is a block diagram showing the arrangement of the endoscope image sensing apparatus according to  
15 the first embodiment of the present invention. The first embodiment is characterized in that a CPU 31 reads out coefficients of a predetermined color matrix from a table of a ROM 35 on the basis of the operation of a switch 34 by the user, and perform predetermined  
20 image processing for color reproduction on the basis of the color matrix coefficients. This characteristic feature will be described in detail below.

As shown in FIG. 2, a CCU 5 incorporates a CCD driver 13 for driving/controlling a CCD 11. The CCD  
25 driver 13 supplies a CCD driving signal to the CCD 11 through a CCD driving signal transmission line in a camera cable 12. The signal charge stored in the CCD

11 is read out as a CCD output signal.

The CCD output signal read out from the CCD 11 is amplified by a preamplifier 14 and sent to the CCU 5 through a CCD output signal transmission line in the camera cable 12. This signal is input to a preprocess circuit 15 in the CCU 5.

An A/D conversion circuit 16, isolation circuit (to be abbreviated to I. L hereinafter) 17, and Y/C separation circuit 18 are connected to the output stage of the preprocess circuit 15. The CCD output signal input to the preprocess circuit 15 is subjected to preprocesses such as CDS (Correlation Double Sampling) and S/H (Sampling/Holding). The resultant signal is input to the A/D conversion circuit 16 to be converted into a digital signal. This digital signal is electrically isolated by the I. L 17 and input to the Y/C separation circuit 18.

A color difference LPF (Low-Pass Filter) 19, a line-sequential format circuit 20, and a color separation circuit 21 constituted by an RGB matrix are connected to the output stage of the Y/C separation circuit 18. The digital signal input to the Y/C separation circuit 18 is separated into the luminance signal Y and the chromatic signal C. Pseudo color components and the like are removed from the chromatic signal C by the color difference LPF 19 and the signal is converted into line-sequential signals by the

line-sequential format circuit 20. As a consequence, three digital signals Y, Cr, and Cb are input to the color separation circuit 21. These signals are converted into R, G, and B digital signals by the color separation circuit 21.

When the above digital signals Y, Cr, and Cb of the three systems are to be converted into the R, G, and B signals, the CPU 31 reads out corresponding coefficients (color matrix) from the table held beforehand in the ROM 35 in accordance with an operation command from the switch 34 operated by the user, and performs a predetermined arithmetic operation for realizing desired color reproduction. This operation is a characteristic feature of the present invention and will be described in detail later.

An AGC & painting circuit 22, exposure control circuit 24, and knee &  $\gamma$  correction circuit 23 are connected to the output stage of the color separation circuit 21. The R, G, and B signals from the color separation circuit 21 are subjected to gain adjustment and painting processing in the AGC & painting circuit 22. The resultant signals undergo exposure control processing in the exposure control circuit 24. The knee &  $\gamma$  correction circuit 23 then performs knee processing and nonlinear  $\gamma$  correction processing to compress the information of the high-luminance portion of each signal.

For example, a digital signal (input) consisting of 11-bit data and input from the input stage is compressed into an 8-bit digital signal (output) by the knee processing and  $\gamma$  processing in the knee &  $\gamma$  correction circuit 23. An encoder 25 is connected to the output stage of the knee &  $\gamma$  correction circuit 23 to convert each signal into a standard TV signal, e.g., an NTSC signal. This signal is impedance-matched by a 75- $\Omega$  driver 26 and output to a TV monitor 6.

The CCU 5 has a reference signal generating circuit (to be abbreviated to SSG hereinafter) 27. A timing signal generating circuit (to be abbreviated to TG hereinafter) 29 generates various timing signals to the respective circuits described above on the basis of the reference clock signals generated by the SSG 27 and electrically isolated by an I. L 28.

The CCU 5 also includes a detection circuit 30 for detecting the brightness of an image based on the R, G, and B signals from the color separation circuit 21.

The detection output from this detection circuit 30 is output to the CPU 31. The CPU 31 then checks whether the brightness of the image is equal to or higher than a predetermined level, and controls a peripheral interface (to be referred to as a peripheral I/F hereinafter) 32 on the basis of the brightness of the image. As a consequence, the peripheral I/F 32 outputs a setting signal and control signal to the exposure



control circuit 24 and CCD driver 13.

5 The control signal from the peripheral I/F 32 to the CCD driver 13 is electrically isolated by an I. L 33. These I. Ls 17, 28, and 33 are used to secure safety by electrically isolating the scope 3 side from the CCU 5 side because the endoscope image sensing apparatus 1 is a medical device.

10 The exposure control circuit 24 is comprised of first and second coefficient registers for receiving a field signal from the TG 29 and a setting signal from the peripheral I/F 32 controlled by the CPU 31, discriminating a 1-field period on the basis of an edge of the field signal, and outputting a coefficient signal corresponding to the setting signal from the peripheral I/F 32 in synchronism with each 1-field period, a first multiplier for multiplying each of 11-bit R, G, and B digital signals received through the AGC & painting circuit 22 by the coefficient signal from the first coefficient register, a delay circuit 15 having a field memory for delaying each of the R, G, and B digital signals received through the AGC & painting circuit 22 by a 1-field period, and a second multiplier for multiplying each of the R, G, and B digital signals, delayed by the delay circuit by 20 a 1-field period, by the coefficient signal from the second coefficient register. The exposure control circuit 24 is comprised of an adder for adding the 25

outputs from the first and second multipliers, a delay circuit for delaying the output from the adder by a 1-field period, and an interpolation circuit for interpolating the output from the delay circuit.

5           The first embodiment having the above arrangement is characterized in that a color matrix to be used for conversion of the three digital signals Y, Cr, and Cb into the R, G, and B digital signals in the color separation circuit 21 can be selected on the basis of  
10           the operation of the switch 34 by the user.

          More specifically, when the user operates the switch 34, the CPU 31 reads out the color matrix corresponding to the operation command by referring to the table held beforehand in the ROM 35, and outputs  
15           the color matrix to the color separation circuit 21, thereby performing predetermined arithmetic processing.

          FIG. 3 shows the detailed arrangement of the color separation circuit 21.

          The color separation circuit 21 includes a CPU  
20           interface 51 for receiving an input from the CPU 31, a coefficient register 52 for holding the color matrix coefficients sent from the CPU 31, an input register 50 for holding signals from the Y/C separation circuit 18 and the like, and an output register 55 for holding the  
25           operation result obtained by performing a predetermined arithmetic operation based on the coefficients held by the coefficient register 52 using multipliers 53a to

53i and adders 54a to 54c.

According to this arrangement, a matrix operation is:

$$\begin{pmatrix} R \\ G \\ B \end{pmatrix} = \begin{pmatrix} k11 & k12 & k13 \\ k21 & k22 & k23 \\ k31 & k32 & k33 \end{pmatrix} \begin{pmatrix} Y \\ R - Y \\ B - Y \end{pmatrix}$$

5 This arithmetic operation attains processing that realizes color reproduction independent of the light source to be used, together with general white balance processing.

10 In the first embodiment, the user can select suitable one of the above color matrixes in accordance with the observation region and the type of light source to be used by operating the switch 34. This makes it possible to realize color reproduction desired by the user.

15 The second embodiment of the present invention will be described next.

FIG. 4 shows the arrangement of the endoscope image sensing apparatus according to the second embodiment of the present invention. As shown in  
20 FIG. 4, this endoscope image sensing apparatus is characterized in that a light source section 4 and CPU 31 are connected to each other through a communication section 36 to communicate with each other. In this embodiment, the type of light source can be  
25 discriminated by serial communication.

The second embodiment is characterized in that the CPU 31 receives an identification signal from a light

source by serial communication through the communication section 36, detects the type of light source on the basis of the identification signal, reads out a color matrix corresponding to the type of light  
5 source from a ROM 35, and outputs the matrix to a color separation circuit 21 to perform a predetermined arithmetic operation.

The remaining arrangements and functions are the same as those of the first embodiment, and hence  
10 a repetitive description will be avoided.

With the above processing, in the second embodiment, since a color matrix corresponding to the type of light source is automatically selected, and a predetermined arithmetic operation is performed,  
15 suitable color reproduction can be realized without distinction of the type of light source used, e.g., a halogen lamp, xenon lamp, or metal halide lamp.

The third embodiment of the present invention will be described next.

20 Since the arrangement of the endoscope image sensing apparatus according to the third embodiment is substantially the same as that of the first embodiment, a repetitive description will be avoided, and the characteristic feature of the third embodiment will be  
25 described below with reference to the arrangement in FIG. 2.

The third embodiment is characterized in that the

type of light source is discriminated on the basis of the magnitude of a gain coefficient for white balance, and color matrixes are switched accordingly.

5 In general, since a metal halide light source emits bluish light, the gain value of a red light component becomes large upon white balance adjustment. A halogen light source emits yellowish light. In this case, therefore, the gain value of a blue light component becomes large upon white balance adjustment.

10 In the third embodiment, in consideration of the characteristics of each light source described above, the light source used is discriminated in accordance with the gain value, and color matrixes are switched accordingly.

15 A color matrix switching sequence will be described in detail below with reference to the flow chart of FIG. 5. First of all, arithmetic processing is performed by using color matrix 1. In this case, a CPU 31 reads out color matrix 1 that is held in a ROM  
20 35 assuming the use of a xenon lamp, which is used most widely, and performs predetermined arithmetic processing in a color separation circuit 21 on the basis of color matrix 1 (step S1).

25 The CPU 31 then calculates gain values  $G/R$  and  $B/G$  (step S2). If the gain value  $R/G$  is smaller than a predetermined value  $a$ , since it indicates the gain value of a red light component is large, the CPU 31

determines that a metal halide lamp is used, and reads out color matrix 2 corresponding to the metal halide lamp from the ROM 35 (step S4). The CPU 31 then performs predetermined arithmetic processing in the color separation circuit 21 on the basis of color matrix 2 (step S5). The CPU 31 computes the gain values R/G and B/G again (step S6).

If the gain value B/G is smaller than a predetermined value  $\underline{b}$  (step S7), since it indicates that the gain value of a blue light component is large, the CPU 31 determines that a halogen lamp is used, and reads out color matrix 3 corresponding to a halogen lamp from the ROM 35 (step S8). The CPU 31 then performs predetermined arithmetic processing in the color separation circuit 21 on the basis of color matrix 3 (step S9). The CPU 31 computes the gain values R/G and B/G again (step S10). In this manner, the CPU 31 performs a predetermined white balance adjustment on the basis of the above gain value (step S11), and then terminates the operation.

A color matrix computation and white balance adjustment for color reproduction are simultaneously implemented by one color separation circuit 21 like the one shown in FIG. 3. If a matrix computation corresponding to a general-purpose light source is performed, the gain coefficient obtained when white balance processing is performed is fed back to the CPU 31.

The CPU 31 then recognizes the light source used in accordance with the gain coefficient. Upon determining that the color matrix is not suitable, the CPU 31 reads out a suitable color matrix from the ROM 35, and the color separation circuit 21 executes a matrix computation again. With the above sequence as an example, color reproduction is realized independently of the type of light source used.

A modification of the first embodiment will be described finally.

FIG. 6 is a block diagram showing the arrangement of an endoscope image sensing apparatus according to a modification of the first embodiment. FIG. 7 shows an example of a display menu.

This modification is characterized in that a monitor 37 for displaying an observation image is connected to the apparatus to display the contents to be selected with the switch 34 are displayed superimposed on the observation image on the monitor 37.

FIG. 7 shows an example of the display, in which display menu [MENU] COLOR MODE 1 is displayed superimposed on the observation image.

According to this modification, since the contents to be selected can be displayed on the screen of the monitor 37, a setting error and the like caused by the user can be prevented.

The embodiments of the present invention have been

described above. However, the present invention is not limited to them, and various changes and modifications can be made without departing from the spirit and scope of the invention. For example, in each embodiment  
5 described above, a one-chip color CCD is used. Obviously, however, a three-chip color CCD can be used. In addition, the metal halide lamp serving as the light source includes an AC metal halide lamp and DC metal halide lamp.

10 The effects of the first to third embodiments will be summarized below.

According to the first embodiment of the present invention, one of the color matrixes stored in the ROM  
35 as a storage means is selected on the basis of the operation of the switch 34 as a designating means  
15 operated by the user, and the CPU 31 as a control means outputs the selected matrix to the color separation circuit 21 as a conversion matrix means. As a consequence, the color separation circuit 21 converts  
20 the luminance and color difference signals into primary color signals.

According to the modification of the first embodiment, since the contents to be selected can be displayed on the screen of the monitor 37 as a display  
25 means, a setting error and the like caused by the user can be prevented.

According to the second embodiment, the CPU 31



as a control means performs serial communication with the light source section 4 through the communication section 36 as a communication means, and recognizes the type of light source on the basis of the identification  
5 signal sent from the light source section 4. Coefficients associated with a color matrix corresponding to the recognized type are read out from the ROM 35 as a storage means and output to the color separation circuit 21 as a conversion matrix means. The luminance  
10 and color difference signals are then converted into primary color signals on the basis of the color matrix.

According to the third embodiment, the CPU 31 as a control means discriminates the type of light source in accordance with the magnitude of the coefficient  
15 used for a white balance adjustment, and reads out coefficients associated with the color matrix corresponding to the type from the ROM 35. The coefficients are output to the color separation circuit 21 as a conversion matrix means, and the luminance and color  
20 difference signals are converted into primary color signals on the basis of the color matrix.

As described above, according to the present invention, first, optimal color reproduction can be realized in accordance with the regions of interest  
25 such as a region with heavy bleeding, a region with a lot of fat, or a substantially white region, e.g., a joint, the technique used, the preference of the user,

or the like. Second, differences in color reproduction due to different types of light sources, e.g., a halogen lamp, xenon lamp, or metal halide lamp, are absorbed to realize consistent color reproduction independent of the types of light sources.

According to the present invention, therefore, there is provided an endoscope image sensing apparatus which can switch suitable color matrixes depending on the type of an observation region, the type of light source used, or the like, and can obtain excellent color reproduction corresponding to the type of observation region or the type of light source used.

Additional advantages and modifications will readily occur to those skilled in the art. Therefore, the invention in its broader aspects is not limited to the specific details and representative embodiments shown and described herein. Accordingly, various modifications may be made without departing from the spirit or scope of the general inventive concept as defined by the appended claims and their equivalents.

WHAT IS CLAIMED IS:

1. An endoscope image sensing apparatus  
comprising:

an image sensing section for obtaining an image  
5 signal by photoelectrically converting an object image;

a conversion matrix section capable of changing  
a setting associated with a conversion matrix to a  
desired setting, the conversion matrix being used to  
convert the image signal, obtained by said image  
10 sensing section, into a video signal, by a predeter-  
mined matrix computation; and

an input section for inputting information about  
a change in the setting associated with the conversion  
matrix.

15 2. An apparatus according to claim 1, wherein  
said conversion matrix section includes a color  
adjustment processing section for performing color  
adjustment processing, and changes a setting associated  
with conversion performed by said conversion matrix  
20 section on the basis of a gain coefficient set when the  
color adjustment processing is performed.

3. An apparatus according to claim 1, wherein  
said image sensing section is a one-chip color CCD, and  
said conversion matrix section converts luminance  
25 and color difference signals into primary color signals.

4. An apparatus according to claim 1, further  
comprising:

a storage section in which a plurality of settings associated with the matrix computation are stored in advance; and

5 a control section for changing the setting by selecting one of the plurality of settings stored in said storage section in accordance with a command from said input section.

5. An apparatus according to claim 4, wherein said image sensing section is a one-chip color CCD, and  
10 said conversion matrix section converts luminance and color difference signals into primary color signals.

6. An apparatus according to claim 4, wherein said conversion matrix section includes a color adjustment processing section for performing color  
15 adjustment processing, and changes a setting associated with conversion performed by said conversion matrix section on the basis of a gain coefficient set when the color adjustment processing is performed.

7. An apparatus according to claim 6, wherein  
20 said image sensing section is a one-chip color CCD, and said conversion matrix section converts luminance and color difference signals into primary color signals.

8. An apparatus according to claim 6, wherein the color adjustment processing is white balance processing,  
25 and said color adjustment processing section is a white balance processing section.

9. An apparatus according to claim 8, wherein

2025061.020400

said image sensing section is a one-chip color CCD, and  
said conversion matrix section converts luminance  
and color difference signals into primary color signals.

10. An endoscope image sensing apparatus  
5 comprising:

an image sensing section for obtaining an image  
signal by photoelectrically converting an object image;

a conversion matrix section for converting the  
image signal obtained by said image sensing section  
10 into a video signal by a predetermined matrix  
computation;

a designating section for designating a change of  
a setting associated with conversion performed by said  
conversion matrix section; and

15 a control section for changing a setting  
associated with the conversion performed by said  
conversion matrix section on the basis of designation  
performed by said designating section.

11. An apparatus according to claim 10, wherein  
20 said designating section is a switching device mounted  
on an operation portion for operating said endoscope  
image sensing apparatus.

12. An apparatus according to claim 10, wherein  
said apparatus further comprises a storage section  
25 in which coefficients associated with the matrix  
computation are stored in advance, and said control  
section reads out a coefficient corresponding to the

designation and stored in said storage section, and outputs the coefficient to said conversion matrix section.

13. An apparatus according to claim 10, wherein  
5 said storage section is a ROM.

14. An endoscope image sensing apparatus comprising:

a light source for irradiating an object with light;

10 an image sensing section for obtaining an image signal by photoelectrically converting an object image;

a conversion matrix section for converting the image signal obtained by said image sensing section into a video signal by a predetermined matrix

15 computation;

a communication section for serially communicating with said light source; and

a control section for performing serial communication with said light source through said communication  
20 section, receiving an identification signal associated with said light source, recognizing a type of said light source, and changing a setting associated with conversion performed by said conversion matrix section on the basis of the type.

25 15. An apparatus according to claim 14, wherein said apparatus further comprises a storage section in which coefficients associated with the matrix

computation are stored in advance, and said control section reads out a coefficient associated with the type of light source from said storage section, and outputs the coefficient to said conversion matrix section.

16. An apparatus according to claim 15, wherein said storage section is a ROM.

17. An endoscope image sensing apparatus comprising:

a light source for irradiating an object with light;

an image sensing section for obtaining an image signal by photoelectrically converting an object image;

a conversion matrix section for converting the image signal obtained by said image sensing section into a video signal by a predetermined matrix computation;

a white balance processing section for performing white balance processing; and

a control section for recognizing a type of light source on the basis of a magnitude of a gain coefficient set when the white balance processing is performed, and changing the setting associated with said conversion matrix section on the basis of the type of light source.

18. An apparatus according to claim 17, wherein said apparatus further comprises a storage section

in which coefficients associated with the matrix computation are stored in advance, and said control section reads out a coefficient corresponding to the type of light source obtained on the basis of a gain  
5 coefficient from said storage section, and outputs the coefficient to said conversion matrix section.

19. An apparatus according to claim 17, wherein said white balance processing section determines gain amounts of red and blue light components on the basis  
10 of results obtained by calculating red of a screen average/green of a screen average and blue of a screen average/green of a screen average.

20. An apparatus according to claim 18, wherein said storage section is a ROM.

15 21. An apparatus according to claim 10, wherein said apparatus further comprises a display section for displaying a setting associated with conversion performed by said conversion matrix section, and when a setting associated with conversion performed by said  
20 conversion matrix section is changed by said designating section, said display section can be referred to.

22. An endoscope image sensing method comprising the steps of:

obtaining an image signal by photoelectrically  
25 converting an object image;

changing a setting associated with a conversion matrix to a desired setting, the conversion matrix



being used to convert the image signal, obtained in the step of performing image sensing, into a video signal, by a predetermined matrix computation; and

inputting information about a change in the setting associated with the conversion matrix.

23. A method according to claim 22, wherein the step of performing conversion matrix processing further comprises the step of performing color adjustment processing, and the method further comprises the step of changing a setting associated with conversion performed in the step of performing conversion matrix processing on the basis of a gain coefficient set when the color adjustment processing is performed.

24. A method according to claim 22, further comprising the steps of:

storing a plurality of settings associated with the matrix computation in advance; and

changing the setting on the basis of a desired setting selected from the plurality of settings stored in said storage section in the step of inputting.

25. A method according to claim 24, wherein the step of performing conversion matrix processing further comprises the step of performing color adjustment processing, and the method further comprises the step of changing a setting associated with conversion performed in the step of performing conversion matrix processing on the basis of a gain coefficient set when

the color adjustment processing is performed.

26. A method according to claim 25, wherein the  
color adjustment processing is white balance processing,  
and the step of performing color adjustment processing  
5 is the step of performing white balance processing.

(100)  
(101)  
(102)  
(103)  
(104)  
(105)  
(106)  
(107)  
(108)  
(109)  
(110)  
(111)  
(112)  
(113)  
(114)  
(115)  
(116)  
(117)  
(118)  
(119)  
(120)  
(121)  
(122)  
(123)  
(124)  
(125)  
(126)  
(127)  
(128)  
(129)  
(130)  
(131)  
(132)  
(133)  
(134)  
(135)  
(136)  
(137)  
(138)  
(139)  
(140)  
(141)  
(142)  
(143)  
(144)  
(145)  
(146)  
(147)  
(148)  
(149)  
(150)  
(151)  
(152)  
(153)  
(154)  
(155)  
(156)  
(157)  
(158)  
(159)  
(160)  
(161)  
(162)  
(163)  
(164)  
(165)  
(166)  
(167)  
(168)  
(169)  
(170)  
(171)  
(172)  
(173)  
(174)  
(175)  
(176)  
(177)  
(178)  
(179)  
(180)  
(181)  
(182)  
(183)  
(184)  
(185)  
(186)  
(187)  
(188)  
(189)  
(190)  
(191)  
(192)  
(193)  
(194)  
(195)  
(196)  
(197)  
(198)  
(199)  
(200)

ABSTRACT OF THE DISCLOSURE

This invention relates to an endoscope image sensing apparatus which can switch suitable color matrixes in accordance with the type of observation region, the type of light source used, or the like, and obtain good color reproduction corresponding to the type of observation region or the type of light source used. This apparatus uses a one-chip color CCD as an image sensing means. A CPU reads out corresponding color matrix coefficients from a ROM, and outputs the coefficients to a color separation circuit. The color separation circuit executes a matrix computation based on the color matrix to convert luminance and color difference signals into primary color signals.

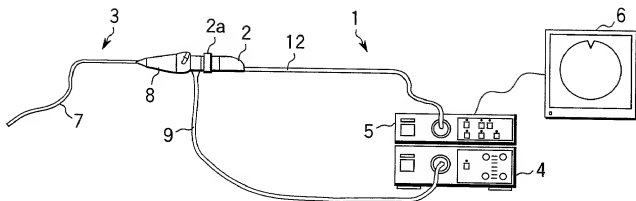


FIG. 1

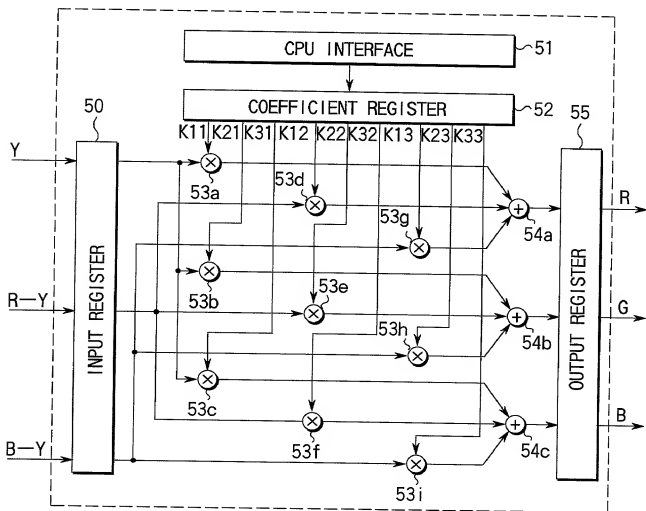
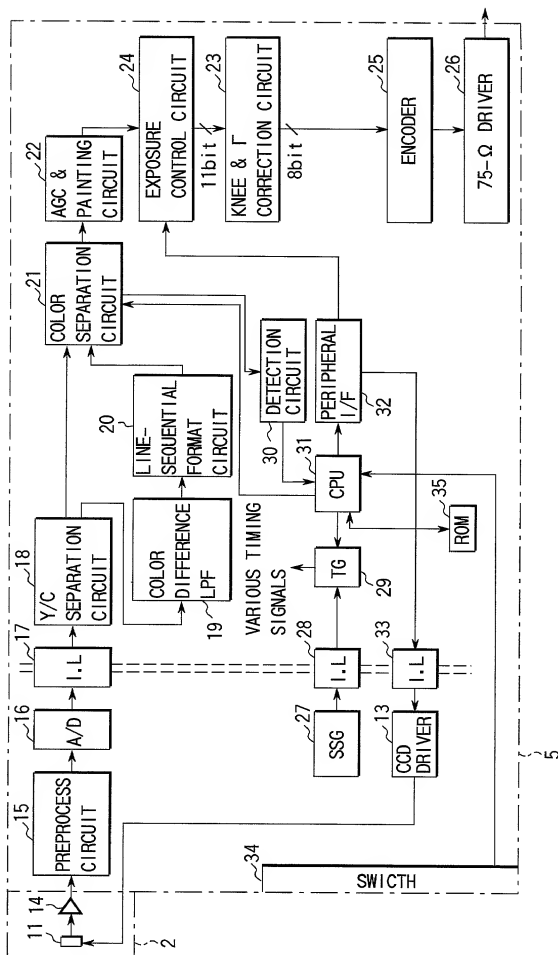


FIG. 3



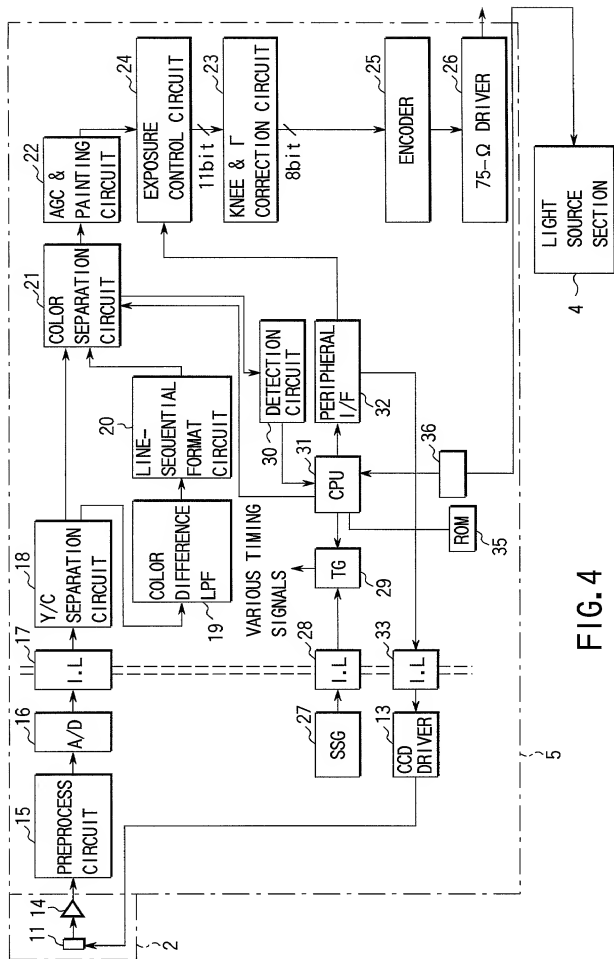


FIG. 4

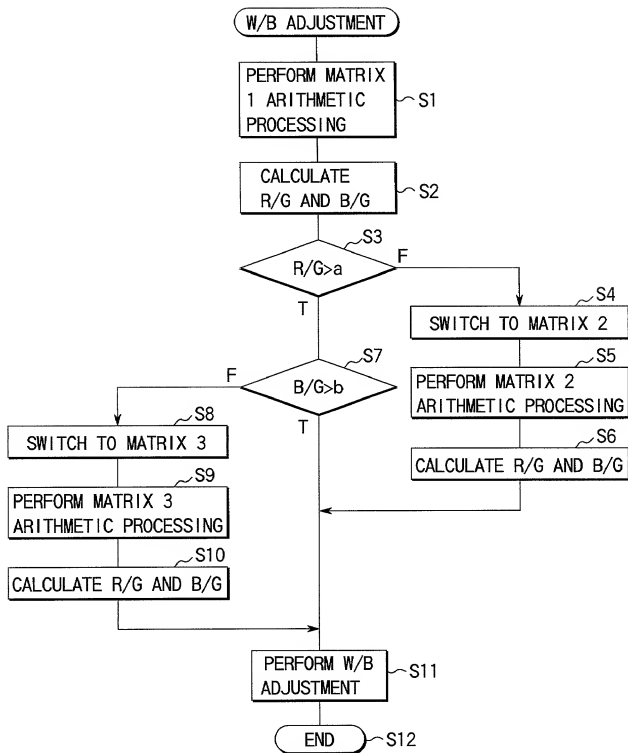
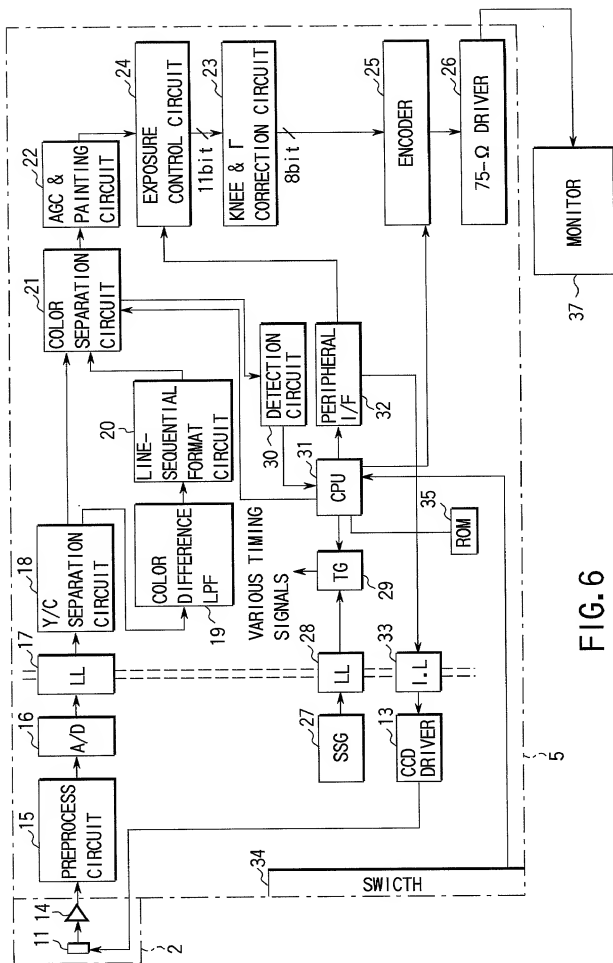


FIG. 5








FIG. 7

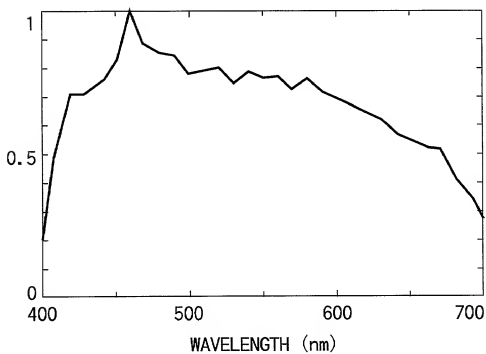
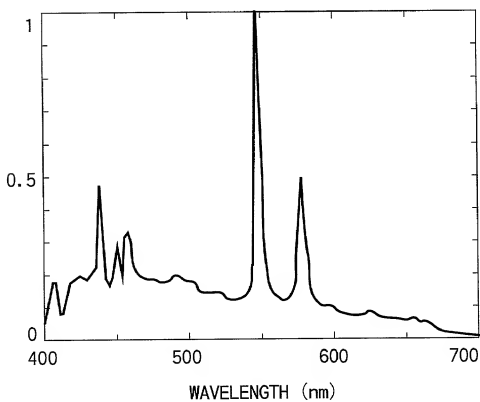
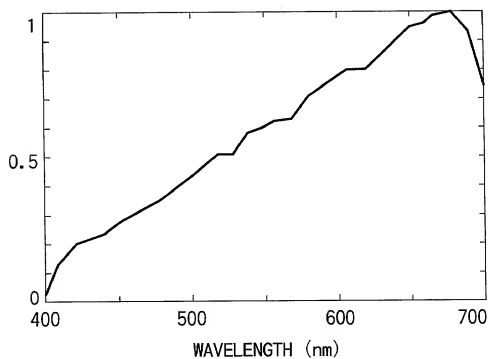


FIG. 8 PRIOR ART



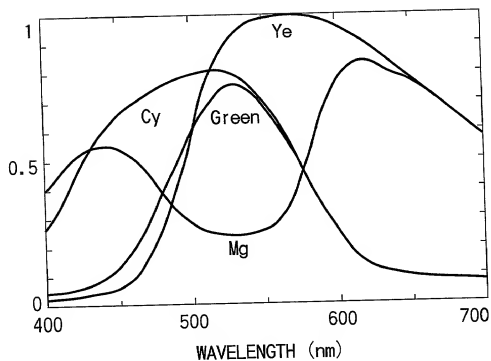


FIG.11 PRIOR ART

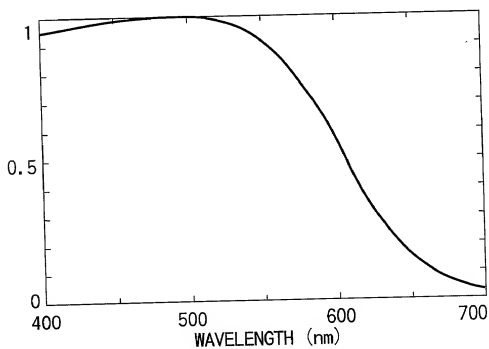


FIG.12 PRIOR ART

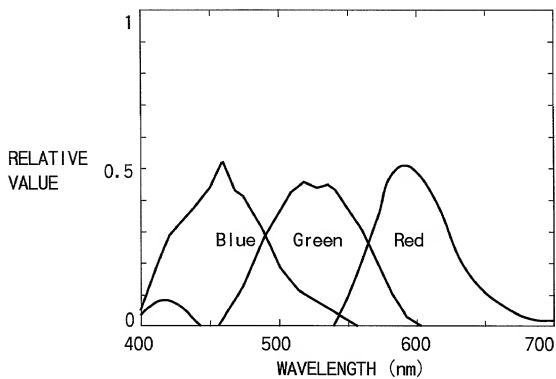


FIG. 13 PRIOR ART

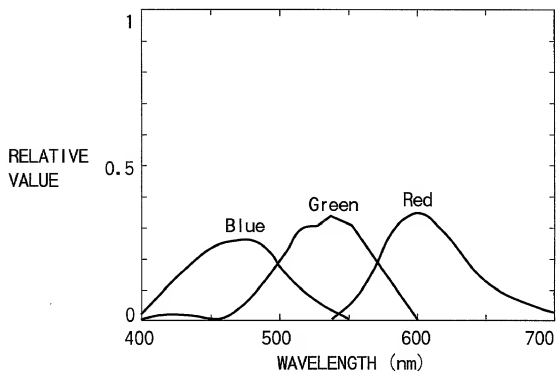


FIG. 14 PRIOR ART

# Declaration Power of Attorney For Patent Application

## 特許出願宣言書及び委任状 Japanese Language Declaration

日本語宣言書

下記の氏名の発明者として、私は以下の通り宣言します。

As a below named inventor, I hereby declare that:

私の住所、私書箱、国籍は下記の私の氏名の横に記載された通りです。

My residence, post office address and citizenship are as stated below next to my name.

下記の名称の発明に関して請求範囲に記載され、特許出願している発明内容について、私が最初かつ唯一の発明者（下記の氏名が一つの場合）もしくは最初かつ共同発明者であると（下記の名称が複数の場合）信じています。

I believe I am the original, first and sole inventor (if only one name is listed below) or an original, first and joint inventor (if plural names are listed below) of the subject matter which is claimed and for which a patent is sought on the invention entitled

内視鏡撮像装置及び内視鏡撮像方法

ENDOSCOPE IMAGE SENSING METHOD  
AND APPARATUS

上記発明の明細書（下記の欄で×印がついていない場合は、本書に添付）は、

The specification of which is attached hereto unless the following box is checked:

☐ \_\_\_\_\_月 \_\_\_\_\_日に  
提出され米国出願番号または特許協定条約

☐ was filed on \_\_\_\_\_  
as United States Application Number or  
PCT International Application Number

国際出願番号を \_\_\_\_\_ とし、  
(該当する場合) \_\_\_\_\_ 月 \_\_\_\_\_ 日に訂正されました。

\_\_\_\_\_ and was amended on  
\_\_\_\_\_ (if applicable).

私は、特許請求範囲を含む上記訂正後の明細書を検討し、内容を理解していることをここに表明します。

I hereby state that I have reviewed and understand the contents of the above identified specification, including the claims, as amended by any amendment referred to above.

私は、連邦規則法典第37編第1条56項に定義されるとおり、特許資格の有無について重要な情報を開示する義務があることを認めます。

I acknowledge the duty to disclose information which is material to patentability as defined in Title 37, Code of Federal Regulations, Section 1.56

# Japanese Language Declaration

(日本語宣言書)

私は、合衆国法典第35編第119条(a)-(d)項又は第365条(b)に基づき下記の、米国以外の国の少なくとも一か国を指定している特許協力条約365(a)項に基づく国際出願、又は外国での特許出願もしくは発明者証の出願についての、外国優先権をここに主張するとともに、優先権を主張している、本出願の前に出願された特許または発明者証の外国出願を以下に、枠内をマークすることで、示しています。

I hereby claim foreign priority under Title 35, United States Code, Section 119(a)-(d) or 365(b) of any foreign application(s) for patent or inventor's certificate, or 365(a) of any PCT international application which designated at least one country other than the United States, listed below and have also identified below by checking the box any foreign application for patent or inventor's certificate, or PCT international application having a filing date before that of the application on which priority is claimed:

Prior Foreign Application(s)

外国での先行出願

Priority Not Claimed

優先権の主張なし

11-027354

JAPAN

04/02/1999

(Number)  
(番号)

(Country)  
(国名)

(Day/Month/Year Filed)  
(出願年月日)

☐

☐

☐

☐

☐

私は、第35編米国法典119条(e)項に基づいて下記の米国外特許出願規定に記載された権利をここに主張いたします。

I hereby claim the benefit under Title 35, United States Code, Section 119(e) of any United States provisional application(s) listed below:

(Application No.)  
(出願番号)

(Filing Date)  
(出願日)

(Application No.)  
(出願番号)

(Filing Date)  
(出願日)

私は、下記の米国法典第35編120条に基づいて下記の米国外特許出願に記載された権利、又は米国外を指定している特許協力条約365条(c)に基づき権利をここに主張します。また、本出願の各請求範囲の内容が米国法典第35編112条第1項又は特許協力条約で規定された方法で先行する米国外特許出願に開示されていない限り、その先行米国外出願書提出日以降で本出願書の日本国内または特許協力条約国際提出日までの期間中に入手された、連邦規則法典第37編1条う6項で定義された特許資格の有無に関する重要な情報について開示義務があることを認識しています。

I hereby claim the benefit under Title 35, United States Code, Section 120 of any United States application(s) or 365(c) of any PCT international application designating the United States, listed below and insofar as the subject matter of each of the claims of this application is not disclosed in the prior United States or PCT information application in the manner provided by the first paragraph of Title 35, United States Code, Section 112. I acknowledge the duty to disclose information which is material to patentability as defined in Title 37, Code of Federal Regulations, Section 1.56 which become available between the filing date of the prior application and the national or PCT international filing date of application:

(Application No.)  
(出願番号)

(Filing Date)  
(出願日)

(Status: Patented, Pending, Abandoned)  
(現況: 特許許可済、係属中、放棄済)

(Application No.)  
(出願番号)

(Filing Date)  
(出願日)

(Status: Patented, Pending, Abandoned)  
(現況: 特許許可済、係属中、放棄済)

私は、私自身の知識に基づいて本宣言書中で私が行う表明が真実であり、かつ私の入手した情報と私の信じることに基づく表明が全て真実であると信じていること、さらに故意になされた虚偽の表明及びそれと同等の行為は米国法典第18編第1001条に基づき、罰金または拘禁、もしくはその両方により処罰されること、そしてそのような故意による虚偽の声明を行えば、出願した、又は既に許可された特許の有効性が失われることを認識し、よってここに上記のごとく宣誓を致します。

I hereby declare that all statements made herein of my own knowledge are true and that all statements made on information and belief are believed to be true; and further that these statements were made with the knowledge that willful false statements and the like so made are punishable by fine or imprisonment, or both, under Section 1001 of Title 18 of the United States Code and that such willful false statements may jeopardize the validity of the application or any patent issued thereon.

039466061-0261100

# Japanese Language Declaration

(日本語宣言書)

委任状: 私は、下記の発明者として、本出願に関する一切の手続きを米特許商標局に対して遂行する弁理士または代理人として、下記の者を指名いたします。  
(弁理士、または代理人の氏名及び登録番号を明記のこと)

POWER OF ATTORNEY: As a named inventor, I hereby appoint the following attorney(s) and/or agent(s) to prosecute this application and transact all business in the Patent and Trademark Office connected therewith. (list name and registration number)

Leonard Holtz (Reg. No. 22,974), Herbert H. Goodman (Reg. No. 17,081),  
Thomas Langer (Reg. No. 27,264), Marshall J. Chick (Reg. No. 26,853),  
Richard S. Barth (Reg. No. 28,180), Douglas Holtz (Reg. No. 33,902), and  
Robert P. Michal (Reg. No. 35,614).

## 書類送付先:

Send Correspondence to  
FRISHAUF, HOLTZ, GOODMAN,  
LANGER & CHICK, P.C.

767 Third Avenue - 25th Floor,  
New York, N.Y. 10017-2023

## 直通電話連絡先:

Direct Telephone Calls to: (name and telephone number)  
Telephone No. (212) 319-4900  
Facsimile No. (212) 644-4834

唯一のまたは第一発明者の氏名	Full name of sole or first inventor
須藤 賢	Masaru Sudo
同発明者の署名 日付	Inventor's signature Date Masaru Sudo Jan. 20, 2000
住所	Residence
日本国八王子市	Hachioji-shi, Japan
国籍	Citizenship
日本	JAPAN
郵便の宛先	Post Office Address
日本国東京都八王子市久保山町2-3	c/o Intellectual Property & Legal Department, OLYMPUS OPTICAL CO., LTD.
オリンパス光学工業株式会社 知的財産法務部内	2-3, Kuboyama-cho, Hachioji-shi, Tokyo, Japan

(第二以降の共同発明者に対しても同様に記載し、署名を  
すること。)

(Supply similar information and signature for second  
and subsequent joint inventors.)

## Japanese Language Declaration

(日本語宣言書)

第 2 共同発明者の氏名 (該当する場合)	Full name of 2nd Joint inventor, if any
松本 勘一	Kanichi Matsumoto
同第 2 発明者の署名 日付	2nd Inventor's signature Date
	<i>Kanichi Matsumoto January 26, 2000</i>
住 所	Residence
アメリカ合衆国、ニューヨーク州 11746、	New York 11746, U. S. A.
国 籍	Citizenship
日本	JAPAN
郵便の宛先 日本国東京都八王子市久保山町 2-3	Post Office Address c/o Intellectual Property & Legal Department, OLYMPUS OPTICAL CO., LTD.
オリンパス光学工業株式会社 知的財産法務部内	2-3, Kuboyama-cho, Hachioji-shi, Tokyo, Japan
第 共同発明者の氏名 (該当する場合)	Full name of Joint inventor, if any
同第 発明者の署名 日付	Inventor's signature Date
住 所	Residence
国 籍	Citizenship
郵便の宛先	Post Office Address
第 共同発明者の氏名 (該当する場合)	Full name of Joint inventor, if any
同第 発明者の署名 日付	Inventor's signature Date
住 所	Residence
国 籍	Citizenship
郵便の宛先	Post Office Address